CX-1 Specifications

Type Digital retinal camera (mydriatic and non-mydriatic)

Types of photography

Retinal observation

Color, FA, Red Free, Cobalt, FAF

Mydriatic: optical viewfinder

Non-mydriatic: camera unit monitor

Angle of view Mydriatic: 50 degrees
Non-mydriatic: 45 degrees

Magnification 2X (Digital)

Minimum pupil size Mydriatic: Ø 5.1 mm or more,

ø 4.3 mm or more when SP function is selected

Non-mydriatic: ø 4.3 mm or more,

ø 3.8 mm or more when SP function is selected

Mounted digital camera Dedicated digital camera by Canon EOS technology

Sensor 15.1 megapixels CMOS

Patient's diopter

compensation range

With "-" compensation lens: -31D to +15D

With "-" compensation lens: -31D to -7D

With "+" compensation lens: -11D to +33D

Working distance

35 mm from the front of objective lens

Working distance adjustment Working distance dots on retina

Fixation target Mydriatic: external type (Standard), internal type (Optional)

Non-mydriatic: internal fixation target (LED dot matrix, green)

Light source Mydriatic: halogen lamp for observation, xenon tube for photography

Non-mydriatic: IRED for observation, xenon tube for photography

Range of base movement 65 mm front and back, 110 mm side to side, 30 mm up and down

Panning range 30 degrees to the right and left
Tilting range 15 degrees up, 10 degrees down
Operating environment Temperature: 10°C to 35°C
Humidity: 30% RH to 80% RH

Dimensions (W x D x H) 320 mm x 531 mm x 577 mm (12.6 in. x 20.9 in. x 22.3 in.)

Weight Approx. 26 kg (57 lbs.)

COMPONENTS

Main unit
Digital camera

External eye fixation lamp

Video cable

Power cable

Camera mount cap

Chin rest paper (100 sheets)

Dust cover

Retinal imaging control software for CX-1

OPTIONAL ACCESSORIES

Stereo unit SU-1

Internal eye fixation CX-IF Chin rest paper (500 sheets)

Simulated images and specifications are subject to change without notice.



CANON INC

MEDICAL EQUIPMENT GROUP

30-2, Shimomaruko 3-chome, Ohta-ku, Tokyo 146-8501, Japan Telephone: +81-3-3757-8497 Fax: +81-3-5482-3960

CANON U.S.A., Inc. Medical Systems Division

15955 Alton Parkway, Irvine, CA 92618-3731, U.S.A. Telephone: (1) 949-753-4160, toll-free within U.S.A.: 1-800-970-7227 Fax: (1) 949-753-4184 http://www.usa.canon.com/eye-care

CANON EUROPA N.V. Medical Systems Division

Bovenkerkerweg 59-61, 1185 XB Amstelveen, The Netherlands Telephone: +31-(0) 20-545-8926 Fax: +31-(0) 20-545-8220 http://www.canon-europe.com/Medical

CANON SINGAPORE PTE. LTD. Medical Equipment Dept.

1 HarbourFront Avenue, #04-01 Keppel Bay Tower, Singapore 098632 Telephone: +65-6796-3549 Fax: +65-6271-4226 http://www.canon-asia.com

CANON (CHINA) CO, LTD. Medical System Division

15F Jinbao Building No.89 Jinbao Street, Dongcheng District, Beijing 100005, China

Telephone: (86) 10-8513-9999 Fax: (86) 10-8513-9914 http://www.canon.com.cn

CANON AUSTRALIA PTY. LTD. Optical Division

1 Thomas Holt Drive, North Ryde, Sydney, NSW 2113, Australia Telephone: +61-2-9805-2000 Fax: +61-2-9805-2444 http://www.canon.com.au/default.aspx








Sleek & Compact. Simple to Operate. Smart. REDEFINING TRUE VERSATILITY

The CX-1 digital retinal camera synergizes digital mydriatic and non-mydriatic imaging capabilities, as well as multiple functions and photography modes – including one-shot FAF photography – by dedicated onboard SLR technology, all in one easy-to-use system.

Code: 0136W333 © CANON INC. 2009 0809SZ0 PRINTED IN JAPAN

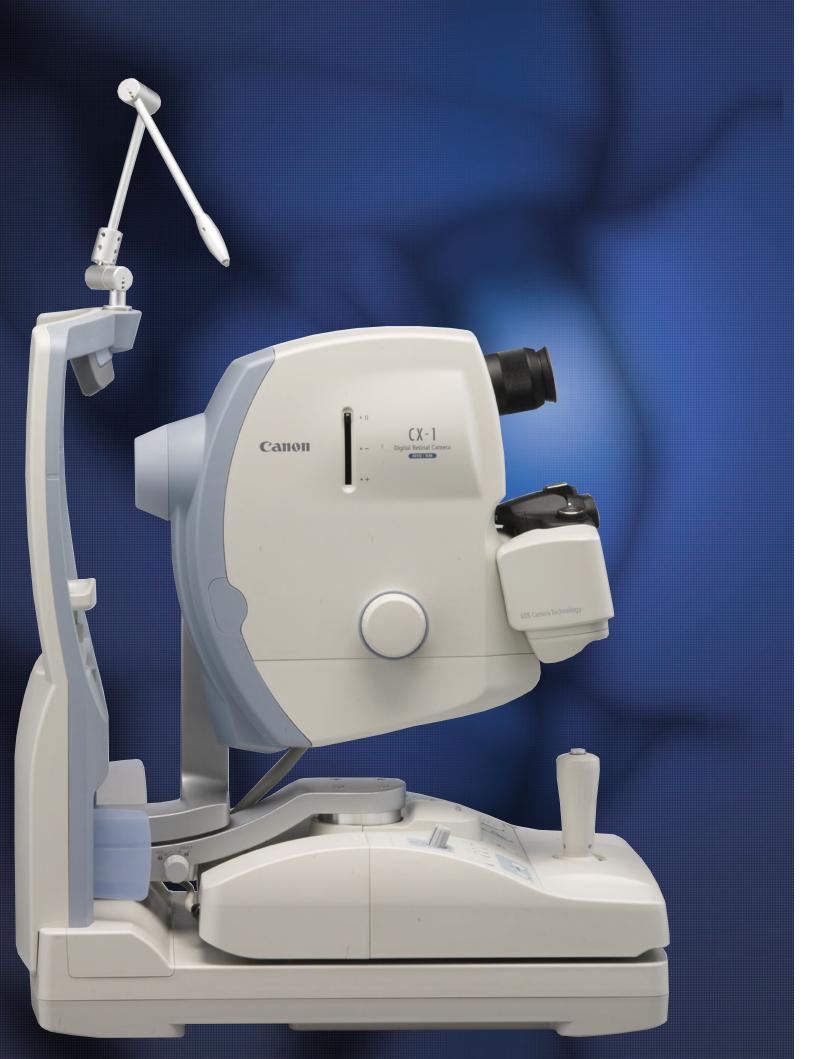



- Myd and Non-Myd hybrid digital retinal camera
- Sleek and compact
- Simple to operate
- Five photography modes (Color, FA, Red-free, Cobalt, FAF)
- One-shot FAF for Myd and Non-Myd
- Advanced stereo photography system
- EOS camera technology for unsurpassed Canon imaging


A CANON INNOVATION – COMBINING MYD & NON-MYD TECHNOLOGIES IN ONE SIMPLE DIGITAL SYSTEM

The CX-1 Digital Retinal Camera is a fully digital hybrid retinal camera system with mydriatic and non-mydriatic modes. High-quality diagnostic image capturing is easier and more efficient than ever. By simple push-button operation, change modes and adjust functions to deliver comfortable procedures to the patient for concurrent eye examinations.



Unprecedented Operation and Functionality















FAF photography

Color photography

Red-free photography

Fluorescein angiography

Five available photography modes.

One-touch selection of Myd/Non-Myd



A Canon first – with one touch, switch between mydriatic and non-mydriatic imaging modes. A single push of the "Myd/Non-Myd" button initiates the automatic adjustment of the inner mechanisms. The operator

can effortlessly utilize different functions within seconds and perform several concurrent ocular tests.

Superior image quality




High-precision Canon optics achieve retinal imaging of the highest quality. Wide angles of view for both Myd and Non-Myd observation are exceptionally clear with higher resolution,

even when magnified to double the original size using "2x Mode."

Intelligent monitor assistance

The onboard EOS camera's LCD monitor provides several

features to assist in efficient image acquisition, such as automatic magnification during focusing for clear split line observation. Magnification size options for the monitor enhance effective examination.




Intuitive operation



The configuration of the controls is based on simplified operation, workflow efficiency, and ergonomic design. During either Myd or Non-Myd observation, select freely from the five available shooting modes for optimal exam combinations. The entire control panel facilitates smooth procedural transitioning; where several steps were once required manually, the CX-1 needs only the touch of a button for

adjustments to occur. The bundled control software provides even further usability.









Screening Revolutionized: Myd & Non-Myd Fundus Autofluorescence


Take Myd or Non-Myd FAF photography as a part of your regular retinal exam. Sharp and clear images. No additional options needed.



FAF photography with Myd and Non-Myd Optimal imaging, even with cataracts **Superior high-quality images**



Sample FAF images with CX-1

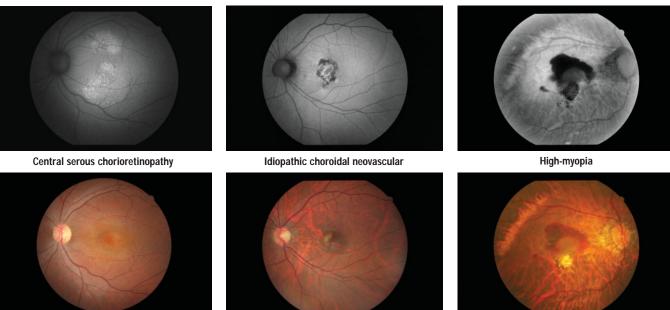

Photos courtesy of Dr. Takayuki Tanaka, Tanaka Ganka lin

What is FAF?

Fundus autofluorescence, or FAF, is the occurrence of autofluorescence in macular waste, particularly Lipofuscin. Examinations that check for and monitor autofluorescent waste material are a key step in AMD detection.



EOS CAMERA TECHNOLOGY

Linking EOS camera technology with CX-1 retinal imaging capabilities for exceptional performance and quality

Canon's own EOS camera technology, with its renowned image processing capabilities, is adapted exclusively for medical use in CX-1 to provide optimal retinal imaging in a compact and convenient system. The single onboard digital camera handles with ease five different photography modes, including nonmydriatic FAF photography, allowing EOS imaging technology to benefit all retinal images from CX-1.

